Artificial Intelligence formulated this projection for compatibility purposes from the original article published at Global Journals. However, this technology is currently in beta. Therefore, kindly ignore odd layouts, missed formulae, text, tables, or figures.

Modeling And Implementing RFID Enabled Operating 1 Environment For Patient Safety Enhancement 2 Dr. Chuan-Jun Su 3 Received: 13 February 2010 Accepted: 4 March 2010 Published: 15 March 2010 л

Abstract 6

Patient safety has become a growing concern in health care. The U.S. Institute of Medicine 7 (IOM) report ?To Err Is Human: Building a Safer Health System? in 1999 included 8 estimations that medical error is the eighth leading cause of death in the United States and 9 results in up to 100,000 deaths annually. However, many adverse events and errors occur in 10 surgical practice. Within all kinds of surgical adverse events, wrong-side/wrong-site, 11 wrong-procedure, and wrong- patient adverse events are the most devastating, unacceptable, 12 and often result in litigation. Much literature claims that systems must be put in place to 13 render it essentially impossible or at least extremely difficult for human error to cause harm to 14 patients. Hence, this research aims to develop a prototype system based on active RFID that 15 detects and prevents errors in the OR. To fully comprehend the operating room (OR) process, 16 multiple rounds of on site discussions were conducted. IDEF0 models were subsequently 17 constructed for identifying the opportunity of improvement and performing before-after 18 analysis. Based on the analysis, the architecture of the proposed RFID-based OR system was 19 developed. An on-site survey conducted subsequently for better understanding the hardware 20 requirement will then be illustrated. Finally, an RFID-enhanced system based on both the 21 proposed architecture and test results was developed for gaining better control and improving 22 the safety level of the surgical operations. 23

24

Index terms— Radio Frequency Identification (RFID), Patient Safety, Operating Room, IDEF0. 25

I. INTRODUCTION 1 26

he Operating Room (OR) briefing is a tool to enhance communication among the team members of operating room 27 and improve patient safety [1], which is the most important and uncompromised issue for medical institutions. 28 It has become a growing concern in health care. As expected, many adverse events and errors occur in surgical 29 practice. Taking the correct patient into the correct OR and executing correct procedures by correct medical staff 30 have become widely understood as the fundamental infrastructure of safe patient care to avoid adverse events in 31 the operating room. Hence, there are four critical requirements to give the right treatment to the right patient: 32 i. Correct patient ii. 33

34 Correct OR iii.

35 Correct medical staff iv.

36 Correct operations Whether wrong patient, wrong location, wrong medical staff or wrong operation event has resulted in injury or didn't raise actual harm, those kind of events cause anxiety for patients and staff, disrupt 37 the smooth flow of patients through the OR suite, and increase the probability of medical errors. Hence, this 38 research aims to develop a prototype system based on RFID that detects and prevents errors in the OR. The 39 system provides hospitals to correctly identify surgical patients and track their operations to ensure they get the 40 correct operations at the right time. 41 II.

42

43 2 LITERATURE REVIEW

Patient safety means minimizing harm to patients arising from medical treatment [2] and is becoming a growing concern in health care. There are many factors involved in patient safety today, and there are many factors to consider when improving the safety process [3]. Recent attention to this topic stems from several high-profile medical errors and several Institute of Medicine (IOM) reports which quantified the problem, created standardized definitions, and charged the healthcare community to develop improved hospital operating systems [4,5].

The operating room (OR) is one of the most complex work environments in health care. Compared with 49 other hospital settings, errors in the operating room can be particularly catastrophic and, in some cases, can 50 result in high-profile consequences for a surgeon and an institution. In addition, the high rate of adverse events 51 in surgery is incessantly demonstrated. According to a sentinel event alert issued ??ec 5, 2001, by the Joint 52 Commission on Accreditation of Healthcare Organizations (JCAHO), "fifty-eight percent of the cases occurred 53 in either a hospital-based ambulatory surgery unit or freestanding ambulatory setting, with 29 percent occurring 54 in the inpatient operating room and 13 percent in other inpatient sites such as the Emergency Department or 55 ICU. Seventy-six percent involved surgery on the wrong body part or site; 13 percent involved surgery on the 56 wrong body part or site; and 11 percent involved the wrong surgical procedure" [6]. After the astonishing report 57 published by ??CAHO Gawande et al., in 2003, analyzed errors reported by surgeons at three teaching hospitals 58 and found that seventy-seven percent involved injuries related to an operation or other invasive intervention 59 (visceral injuries, bleeding, and wound infection/dehiscence were the most common subtypes), 13% involved 60 unnecessary or inappropriate procedures, and 10% involved unnecessary advancement of disease. In addition, 61 two thirds of the T incidents involved errors during the intra-operative phase of surgical care, 27% during 62 pre-operative management, and 22% during post-operative management [7]. In other words, no matter how 63 well-trained a medical staff is, he or she could still make mistakes. Within all kinds of surgical adverse events, 64 wrong-side/wrong-site, wrong-procedure, and wrong-patient adverse events (WSPEs) are the most devastating, 65 unacceptable, and often result in litigation. However, an estimate of 1300 to 2700 WSPEs per year based on the 66 available databases, extensive review of the literature, and discussion with regulators in the United States seems 67 likely [8]. A variety of studies have demonstrated that the rates of adverse events associated with surgery are 68 substantial. Of course, surgery inherently carries risk, and only 17 per cent of these adverse events were judged 69 to be preventable [9]. Nonetheless, this important proportion of surgical adverse events is preventable given what 70 is known today. Systems must be put in place to render it essentially impossible or at least extremely difficult 71 for human error to cause harm to patients. With the introduction of new approaches many other complications 72 that are not associated with an obvious error may be preventable in the future. 73

74 III.

75 **3 REQUIREMENT STUDY**

76 As mentioned in the previous chapters, the high rate of sentinel events in surgery has been incessantly 77 demonstrated. Among all sentinel events, performing a procedure on the wrong site or the wrong patient is mostly preventable and should never happen. Much literature claims that systems must be put in place to 78 render it essentially impossible or at least extremely difficult for human error to cause harm to patients. Among 79 a lot of novel technologies, RFID is an enabling technology that is generally considered to improve patient 80 safety and savings in hospital. This technology has been applied for many fields but few applications specified 81 to OR. Moreover, little literature analyzed from the business processes' point of view to reap the benefits of 82 RFID but focus on an object or an individual. Therefore, we proposed using RFID from the processes' point of 83 view to detect errors that may lead to wrong site or the wrong patient surgery. Before an RFID implantation, 84 opportunity survey based on business process analysis is necessary. The survey consists of the following phases: 85 Expert interview and site survey-Expert interview and site survey have conducted to comprehend the process in 86 OR. 87

Existing OR Process: Based on the result of expert interview and site survey, we described the existing OR process. IDEF0 modeling-: IDEF0 modeling technique is adopted to (1) build the OR as-is model based on the result of previous step, (2) analyze the activities in the previous OR process.

91 4 RFID-based OR Process:

Based on the results of previous steps, we described an RFID-based state for the process.

⁹³ 5 A. Expert Interview and Site Survey

Before an RFID implantation, opportunity survey based on business process analysis is necessary. This experience
can also be applied in a hospital. Surgeons, nurses and anesthetists are the experts who know what happens
behind the closed doors of the operating department. They clearly know their job functions and workflow during

97 surgery. For this reason, we undertook several expert interviews with the medical staff worked in an operating 98 department of a regional teaching hospital in Taoyuan to comprehend the operative process. Except expert

⁹⁹ interviews, we also perform site survey to observe the activities in OR.

The activities during on-site survey include observation of nursing work, review related forms and face-to-face meeting with nurses to capture the entire workflow in OR. The results of expert interviews and on-site survey are described in the following sections.

¹⁰³ 6 B. Expert Interview And Site Survey

The scope of OR process for an individual patient which we describe as follows begins with the surgical patient's 104 arrival at the OR suite and ends when the patient leaves the OR suite. The details of the OR process is shown 105 below: Admission into operating suite-Base on operations schedule, the transporter brings scheduled surgical 106 patient from ward to the operating suite, along with his/her medical record and related document. Upon the 107 patient's arrival in the holding area of operating suite, the holding area nurse orally identifies patient by matching 108 the replies from the patient about the name, ID card number, type of surgery with medical record, etc. After the 109 confirmation, the nurse reviews the document accompanying the patient to check whether the operation related 110 forms such as operative consent form has been completely filled in or not. The patient's national health insurance 111 card is then received by the nurse. After a series of admission procedure, the nurse logged on to the hospital 112 information system to change the patient's status. At the same time, the patient's status information -Wait ing 113 for surgery? is displayed in the screen located in the waiting area to reduce anxiety patient's family members. 114

Admission into operating room-The surgical patient stays in the pre-operative holding area until the OR is ready. However, before a circulating nurse takes a patient into scheduled OR, the nurse verbally identifies the patient again and changes the patient's status from -W aiting for surgery -t o -I n surgery?.

Beginning of anesthesia-The anesthetist verbally confirms the patient's identification, type of surgery and part 118 of surgery before anesthesia. If the information is correct, the anesthetist signs in the nursing records of patients' 119 operations. Although the doctor has already determined the anesthetics and methods of delivery before surgery, 120 the anesthetist can make the final decision depending on the patient's specific condition at that point of time. 121 The anesthetist verbally asks the patient's information such as the history of allergy, family history in the OR 122 to decide which kind of anesthetics he or she should use. Besides, anesthesia staff also reviews the anesthesia 123 information and laboratory test data in medical record to assist determining the way to induce anesthesia is 124 suitable for the patient or not. 125

Surgery-A surgeon also has to confirm the patient's identification before surgery. However, the surgical patient is usually covered with surgical drapes and has been anesthetized when a surgeon enters the OR. The surgeon can only justify the patient by medical record or pictures such as X-ray pictures. In the case that the patient was not covered with surgical drapes, the surgeon verifies patient by face.

Because surgeons often meet surgical patients before surgery, the surgeons consider that they can distinguish a right patient from a wrong patient by their memory. Before performing an operation, the surgeon refers to the patient's medical record to make sure the surgical procedure and the site of operation. During surgery, surgeon can refer to medical record for the anesthesia information, patient information, results from laboratory information system if necessary. In the operating room information about the location of equipment had direct and sometimes critical implications for patients' clinical outcomes [8].

Admission to recovery-After surgery the patient is takes into recovery rooms to wait for "awakening" from anesthesia. At the same time, the nurse in the recovery room changes the patient's status to? In recovery?.

Discharge from operating suite: After a patient becomes conscious, the transporter takes the patient back to his/her ward and change patient's status information to -R eturn ward?.

¹⁴⁰ 7 C. IDEF0 Modeling

After in-depth understanding of the current process in OR an IDEF0 model was developed. The IDEF0 model 141 is used to help organizing the analysis of OR system and to promote good communication between the analyst 142 and the medical staff. For better understanding of the sequence, we chose sequential form of breakdown which 143 decomposes the parent activity by a sequence of sub-activities to build our system. However, the structure 144 imposed by the IDEF0 methodology naturally creates a set of questions that must be asked and answered about 145 each function and its sub-functions. The answers to these questions provide important information concerning 146 how known human fallibilities which may lead to errors. Thus, we can clarify many activities during model 147 development stage by discussing with medical staff. In this section, first, we built the -as -is? model to define 148 activities and functions in OR. The definition of -as -is? is a description of the current situation in terms of the 149 work processes. With sufficient information regarding the as-is operation, analyzing current process and building 150 a new system become easier. Second, we examined the model, found out the operations which probably threaten 151 to patient safety or make medical staff ineffective and analyzed the opportunity for introducing RFID to solve 152 the problem. 153

¹⁵⁴ 8 D. Building "as-is" Model

After expert interviews and on-site survey, the OR as-is model was constructed. The purpose of this model is to find out the systemic vulnerabilities that may lead to human error and the opportunities that can improve medical staff's operations by introducing RFID technology. The model was developed from the OR medical staff's viewpoint. Fig. ?? depicts the top-level function of the IDEF0 model, -perform surgery?. The activity called -perf orming surgery? is broadly defined as all activities during per-, intra-and post operations. Fig. ?? shows the top-level function decomposed into six more specific functions, representing the surgery process in more detail. Note that the general inputs, outputs, controls, and mechanisms from Fig. ?? are also decomposed, illustrating the progressive exposure of detail that is a feature of the IDEF0 methodology; Fig. ?? shows the decomposition of the activity -pati ent check-in? at an even higher level of detail. In the same way, Fig. ??, 5 and 6 shows the decomposition of the other activities in detail.

¹⁶⁵ 9 E. As-is Model Analysis and RFID Solutions

In the operating room information about the location of equipment had direct and sometimes critical implications 166 for patients' clinical outcomes [10]. After building the OR as-is model and numbers of meeting with related 167 medical personnel, we discovered that there were a lot of systemic vulnerabilities that may lead to human 168 error. In real situations, not every OR member completely follows the Standard Operating Procedures (SOP). If 169 some accidental situations happen, wrong patient, wrong site/side surgery, unsuitable anesthesia or wrong OR 170 171 event may occur. Based on the as-is model, the possible human errors and inefficient operations are listed as 172 follows: Inducing unsuitable anesthesia-An anesthetist has to make the final decision regarding the anesthetics and methods of delivery at the time of surgery. Therefore, providing sufficient information to the anesthetist is 173 174 very important. In general, the critical information that aids an anesthetist making decision must be obtained 175 from both ways: verbally asking the patient and reviewing some data described in the medical record. The questions now arise: first, some critical information even was not recorded in a patient's medical record. History 176 of allergy and family history, for example, only can be received by asking patients. If the patient is not conscious 177 or too elderly to answer the questions from medical staff, it would cause the patient to be exposed to danger. 178 Second, looking for the unfiltered data on the paper is inefficient to anesthesia staff. Performing wrong operations-179 Wrong operation mentioned here includes performing wrong procedures on a patient or perform a surgery on the 180 181 wrong site/side of a patient's body. Based on the as-is model, the doctor conforms patient's operation-related 182 information by checking the patient's medical record and surgery-site chart that describes the surgical site/side of a patient. However, because it is not convenient to find out disperse data by looking up the paper-based medical 183 records, doctors sometimes depend on their memory for patients' condition without double-check. In addition, 184 when a surgeon substitutes for another surgeon to perform a surgery or a surgeon operates on more than one 185 patient at the same time, the wrong operation may be performed. 186

Inefficiently updating patient's states-Based on the as-is model, nurses have to manually update a patient's status information (in surgery, in recovery, etc.) in the hospital information system when the patient's status is changed. However, the essence of the OR nurses is to provide care and support to patients before, during, and after surgery. This kind of unrelated activity distracts medical staff and obstructs medical professionals providing better patient care. -Wrong Procedure A42 Passive and inconvenient confirmation processes do not encourage medical staff to reconfirm patient's information. A substitute surgeon is not familiar with the surgical patient. A surgeon operates on more than one patient simultaneously.

-Wrong Anesthesia A41 A patient who is not conscious or too elderly to answer the questions from medical staff causes that some critical information can not be obtained.

196 It is inconvenient to look for dispersed and unfiltered information.

-Inefficient Operations A15, A23, A5, A6 Wasting time to update patients' status information in the computer
 obstructs medical professionals providing better patient care.

As mentioned above, not every OR member completely follows the SOPs in real situations. Therefore, if some 199 200 accidental situations happen, wrong patient, wrong site/side surgery, unsuitable anesthesia or wrong OR event 201 may occur. Table1 shows potential cases that may threaten patient's safety in the as-is model. Human error is inevitable and unavoidable. However, most preventable adverse events are not simply the result of human error 202 but are due to defective systems that allow errors to occur or go undetected. Therefore, we propose an RFID-203 based OR system that can reinforce SOP and prevent potential errors for achieving the ultimate objective of 204 improving patient safety in OR. The proposed RFID-based OR system is expected to complement current human-205 based operations in the following ways: Patient Identification-Improving the accuracy of patient identification is 206 one of JCAHO 2006-2007 patient safety goals which suggest using active communication technique to conduct 207 final verification process and using at least two patient identifiers. However, either suggestion was not adopted 208 in the "as-is" process. The problem can be solved by introducing RFID that can automatically identify patients 209 to complement current human-based verification. Surgical site verification-To decrease the incidence of wrong 210 211 site/side surgery, we have developed a digital chart of surgery site marking which can be displayed on the LCD 212 monitor of OR. By integrating RFID with hospital information system (HIS), the digital chart and some critical 213 information of the patient are automatically shown on the monitor when the patient is brought to the scheduled 214 OR.

OR verification-If a patient is brought to an unscheduled OR, the system will create a warning on the monitor. Thus, the RFID-based system checks the wrong-location event to prevent the potential wrong surgery.

Patient status update-The activity of updating patient's status distracts medical staff from surgery related tasks. In the developed RFID-based system, the status will be updated automatically by integrating RFID with the backend HIS.

220 10 F. RFID-enabled OR Process

After analyzing as-is model, we have developed an RFIDbased prototyping system that detects and prevents errors in the OR. The system provides hospitals to 1) correctly identify surgical patients, 2) track the ORs in which patients and medical staff enter, and 3) furnish critical information to ensure patients get the correct operations at the right time and place. The "to-be" RFID-based OR process derived from analyzing the "as-is" model is illustrated as follows:

Admission into the operating suite-When a surgical patient is scheduled to be operated upon, the nurse in the ward assigns the patient an RFID-embedded wristband encoded with a unique ID. When the surgical patient is brought to the holding area in the OR suite, an RFID reader automatically verifies the identity of the patient. If the details of the patient and operation schedule match, the monitor in the holding area displays some brief information about the patient. Simultaneously, the system automatically changes the patient's status information to -wait ing for surgery? in the database. Then, the patient's status information can be displayed on the screen located in the waiting area that it can helps in reducing the anxiety of his/her family members.

Admission into operating room-The RFID readers in the OR automatically capture the information on the 233 patient's tag to identify him/her upon entering the OR. If the details of the patient and the OR into which 234 he/she has entered match, the screen in the OR displays the patient's information, including his/her name, age, 235 gender, laboratory test data, digital surgery-site chart, and scheduled procedure, by associating the tag's ID 236 number with the patient records stored in the hospital information system. However, if an unscheduled patient 237 enters the OR, the system can alert the medical staff to take the necessary measures in the OR. Thus, unfamiliar 238 faces can be checked with assurance, thereby decreasing the probability of performing the procedure on a wrong 239 patient. Subsequently, the system automatically changes the patient's status information to -i n surgery? after 240 confirming that the correct patient has entered the correct OR. In addition, because the time is automatically 241 recorded, the medical staff does not have to record the time manually. Thus, unfamiliar faces can be checked with 242 assurance, thereby decreasing the probability of performing the procedure on a wrong patient. Subsequently, the 243 244 system automatically changes the patient's status information to -i n surgery? after confirming that the correct patient has entered the correct OR. In addition, because the time is automatically recorded, the medical staff 245 does not have to record the time manually. Initiation of anesthesia: When a tagged anesthetist or nurse enters the 246 room, the system will also ensure that the person has entered the right room, thus preventing medical staff from 247 rushing into the wrong OR and administering inappropriate medical treatment. In addition, information such 248 as the history of allergy, family history, and laboratory test data, which aids the anesthetic team in determining 249 the appropriate anesthetics and method of administration, is displayed on the monitor when the anesthetic team 250 enters the OR. Furthermore, any abnormal values will be marked in red to bring them to the medical staff's 251 attention. Surgery-In the same manner, when a surgeon enters the room, the system will also check whether the 252 person has been assigned to the room, in order to prevent doctors from entering the wrong OR and performing 253 surgery on the wrong person. If the patient has not yet been covered with surgical drapes, the surgeon can 254 reconfirm the patient's identity by matching the patient with a photograph displayed on the screen. In addition, 255 the surgeon is also provided with the patient's critical information on the digital display, rather than having to 256 search for the pertinent information in the documented reports. Thus, bringing all this information together not 257 only saves time but also increases patient safety. The surgeons are encouraged to confirm the patient records 258 through the centralized data displayed on the monitor because of this increased accessibility. In the absence of 259 such a system, doctors would generally depend on their memory, without performing any reconfirmation due to 260 the inconvenience involved. 261

Transfer to recovery-After surgery, patients are transferred to the recovery area. Here, the RFID readers detect the patient's RFID tags and the system automatically changes the patient's status to -i n recovery.? Discharge from operating suite: After a patient recovers from anesthesia, the transporter brought the surgical patient leaving recovery room and returning to ward. At this time, the system automatically updates the patient's status information to -returne d to ward.? IV.

²⁶⁷ 11 THE ARCHITECTURE OF RFID-BASED OR SYSTEM

Beside on the result of the previous section, we proposed an architecture of the RFID-based OR system. The 268 architecture of the RFID-based OR system consists of 1) physically distributed RFID readers, tags, 2) an RFID 269 270 server that processes the data from the readers, 3) several client PCs that run different hospital applications, and 271 4) the hospital information system (HIS) that plays the same role as that of an ERP system in enterprise-level 272 architectures. The RFID server contains a backend database and software called the concentrator that receives 273 the data from RFID readers when the tags are detected. Then, the concentrator checks this data for errors and stores it on an operational database. In our architecture, the concentrator also communicates with other 274 software that implement the application's business logic on client PCs. In addition, the RFID server is connected 275 to the HIS to extract hospital data through an intranet. The architecture of this system is illustrated in Fig. 7. 276 In summary, there are five primary components in the RFID-based OR system: (1) Reader, (2) tag, (3) RFID 277 server, (4) client PCs that manage the client-side applications, and (5) the HIS. 278

²⁷⁹ 12 HIS (Hospital Information

280 13 V. IMPLEMENTATION

²⁸¹ 14 A. RFID Hardware Test and Deployment

282 A -Sit e Survey? is essential for real RFID implementation.

The actual RF coverage, number of readers, their placement and configuration, and system accuracy are greatly dependent on environmental factors. In order to increase the feasibility of the hardware in a clinical environment, we deployed our hardware in an OR suite in a regional teaching hospital in Taoyuan to determine the optimum hardware deployment that fits our test scenario. The test environment was set up in three regions of an OR suite including the holding area, OR-5, and the recovery area. After a series of tests, the result each test scenarios is show as Table ?? and the RF coverage as shown in Fig. 8.

²⁸⁹ 15 Table2. Results of Testing

290 16 Test Scenario Goals Results

²⁹¹ 17 Holding area

The reader located in the holding area steadily detects the investigator's arrival. The tagged investigator must be detected by the reader located in the recovery area while he/she entered the area.

294 18 ?

The reader located in the recovery area cannot detect other patients who passed the recovery area on their way to their scheduled ORs.

297 19 ?

²⁹⁸ The reader also can't detect a patient who walked on the corridor outside the OR suite.

299 20 3

Although part of testing results does not meet our requirement, we can use a system to filter certain unnecessary signals. The solution can be summarized as shown in Table ??.

³⁰² 21 Table3. Solution of Redundant RF Coverage

303 22 Location of readers

304 Solution of exceeded RF signalsHolding Area (Exception 1)

If a patient who has already been detected by the reader located in the holding area is detected again, the application system executed in the holding area will omit the event to avoid the patient check-in twice. Therefore,

the RF coverage can extend beyond the zone of the holding area because the detection of a passerby walking on

the corridor in the OR suite will not be processed again.

³⁰⁹ 23 Recovery Area (Exception 2)

The application system executed in the recovery area supposes a patient who was not detected by any other readers located in the OR suite was a passerby. Hence, if a patient who do not have to undergo an operation passed through the recovery area out of the OR suite and is detected by the reader located in the recovery area, the system will filter the event to avoid mistakenly execute the application.

³¹⁴ 24 B. Two Different Types Of Scenarios

After RFID hardware test and deployment, we have proposed two different types of scenarios: normal and 315 accidental situations. The scenario of normal situations describes the general process during surgery; the scenarios 316 of accidental situations show the unexpected events that may threaten patient's safety. Those scenarios was 317 demonstrated by our system to describe how the RFIDbased OR system prevents errors and improve patient 318 319 safety. Scenario 1: Normal situations-Miss Wang (Shiau-ching Wang, a pseudonym) is admitted to the obstetrics 320 and gynecology department of a teaching hospital for surgery. The bed number of Miss Wang is W06-1. The 321 doctor in charge of Miss Wang logged on to the admission application system to enter some surgical information 322 about Miss Wang and to draw the operation site in detail.

Based on the operations schedule, the holding area nurse telephoned the obstetrics and gynecology floor, identified herself by name, and asked for Miss Wang to be prepared for the operation. After the phone call, the nurse checked Miss Wang's medical records, logged on to the admission application system, and assigned an RFID wristband to her. After a while, the transporter arrived at the obstetrics and gynecology department and New Price Wise Wang form to her applied to the admission application system.

³²⁷ brought Miss Wang from the ward to the operating suite, along with her medical records and related documents.

When Miss Wang entered the holding area of the OR suite, the reader grabbed the tag's ID stored in the RFID 328 wristband. Subsequently, the monitor in the holding area displayed brief information about Miss Wang. The 329 screen located in the waiting area outside the OR suite simultaneously displayed the patient's status information 330 as -wait ing for surgery? to reduce the anxiety of the patient's family members. The holding area nurse completed 331 the admission procedure for Miss Wang, after which Miss Wang remained in the holding area waiting for surgery. 332 After a while, the OR was ready for surgery. A circulating nurse took Miss Wang into the scheduled OR-5. While 333 Miss Wang was brought to OR-5, the reader detected Miss Wang's RFID wristband and the monitor located in 334 that OR displayed Miss Wang's personal and surgery-related information. At the same time, the screen located 335 in the waiting area updated the patient's status information as -i n surgery.? An anesthetist, Dr. Chen, entered 336 the OR, and checked the information that would help him make the final decision regarding the anesthetics and 337 methods of delivery. The surgeon, Dr. Lin, entered OR-5 and reviewed the information displayed on the monitor 338 to reconfirm the patient's surgical procedures. Following these checks, the surgery was performed. After surgery, 339 Miss Wang was brought to the recovery area. 340

The readers in the recovery area detected the RFID wristband worn by Miss Wang. Hence, the monitor in the 341 recovery area displayed brief information about Miss Wang. At the same time, the screen located in the waiting 342 area updated the patient's status information as -i n recovery.? After Miss Wang recovered from the anesthesia, 343 344 the transporter brought her from the recovery room to her ward.

345 While Miss Wang has leaved the recovery room, the screen located in the waiting area updated the patient's 346 status information as -return t o ward.? Demonstration of System Usage Scenario 1-After the decision to perform an operation on Miss Wang, the doctor in charge of Miss Wang logged on to the admission application system 347 (See Fig. ??), pressed the button marked -o peration site mark,? and inputted two identification parameters-the 348 number on the identification card and the bed number-in order to provide some surgical information about Miss 349 Wang and to draw the operation site in detail (See Fig. ??0 and Fig. ??1). After the phone call from the OR, the 350 nurse working in ward 6 checked Miss Wang's medical records, logged on to the admission application system, and 351 assigned an RFID wristband to Miss Wang (See Fig. ??2). Miss Wang entered two identification parameters-the 352 number on the identification card and the bed number-to retrieve Miss Wang's information for double-checking. 353 At the same time, the system automatically checked the operation schedule to confirm Miss Wang's operation. 354 After ensuring that Miss Wang was the correct patient whose name had listed in the operation schedule, the 355 system associated the ID stored in the RFID wristband with the patient's identification in the database. After 356 357 this computerized process, the nurse assigned the RFID wristband to Miss Wang.

Fig.12. Assign tag 25358

364

On Miss Wang's arrival in the holding area of the operating suite, the preoperative application associated the tag's 359 ID propagated from the middleware with the patient's identification and checked the patient's identification with 360 the operation schedule. After confirming Miss Wang's identification, the monitor in the holding area displayed 361 brief information about Miss Wang. Subsequently, the system automatically changed the patient's status to -wait 362 ing for surgery? (See Fig. ??3). 363

$\mathbf{26}$ Fig.13. User interface displayed in the holding area

While Miss Wang was brought to OR-5, the operative application updated Miss Wang's status to -i n surgery? 365 to inform her family about the progress of the operation. At the same time, the system automatically executed 366 the user interface and displayed some information about Miss Wang including personal information, surgical site, 367 diagnosis, operation description, laboratory test data, etc. to avoid fragmented communication and dispersed 368 information (See Fig. ??4 and Fig. 15). 369

Fig.14. User interface displayed in the OR-5 I 27370

The information displayed on the screen can be separated into three parts: basic patient information (helps 371 identify the patient), operative information (ensures correct procedures), and advanced information (supports 372 anesthesia decision). Basic patient information includes the patient's picture, name, ID card number, medical 373 record number, bed number, blood type, sex, age, and birthday. Operative information includes the diagnosis, 374 operation description, and the anesthesia administered by the doctor. Advanced information contains a history 375 of allergy, information of diseases in the family, chronic prescription medicines, and laboratory test data. In 376 addition, abnormal values of certain parameters obtained from laboratory results are marked in red to serve as 377 378 a warning. Miss Wang was taken to the recovery room post surgery. On her arrival in the recovery room, the 379 reader located in that room detected her RFID wristband. Subsequently, the postoperative application displayed 380 brief information about Miss Wang on the monitor, changed Miss Wang's status to -in recovery,? and recorded 381 the arrival time in the database (See Fig. ??6).

After Miss Wang recovered from anesthesia in the recovery room, the transporter brought Miss Wang from 382 the recovery room to her ward. Because Miss Wang had leaved the recovery room, the readers were unable to 383 receive the signal from the patient's tag. Therefore, Miss Wang's information was no longer displayed on the 384 monitor and her status was updated to -ret urn to ward.? In addition, the screen located in the waiting area also 385 updated the patient's status information to -return to ward.? 386

³⁸⁷ 28 Fig.16. User interface displayed in recovery area

Scenario 2: Accidental Situations-As mentioned in chapter3, not every OR member completely follows the SOPs in real situations. Therefore, of some accidental situations happen, wrong-patient, wrong-site/side surgery, unsuitable anesthesia or wrong-OR event may occur. The following scenarios show probable situations that may threaten patient's safety in the as-is model.

Wrong OR Event-Based on the abovementioned scenario (Scenario 1), another patient who was assigned to OR-1 was mistakenly brought to OR-5 by a careless circulating nurse before Ms. Wang was brought to the room. Wrong Side Surgery Event-Based on the abovementioned scenario (Scenario 1), Ms. Wang's attending physician unexpectedly cannot perform the operation due to some reason. Another doctor, Dr. Chen, replaced her attending physician; this doctor was not familiar with the patient's condition. Furthermore, he memorized the wrong side of the operation site and did not check the patient's report.

Wrong Patient Event-Another patient, a woman with a similar name (Shiau-chin Wang, a pseudonym) was also admitted to the obstetrics and gynecology department; however, her operation was planned for the next day. The holding area nurse telephoned the obstetrics and gynecology floor, identified herself by name, and asked for -patient Shiau-chin Wang? (giving no other identifying information).

The nurse on the other end listened to the information, but did not reconfirm; the nurse mistook -S hiau-ching Wang? for -Shia u-chin Wang? informed the actual patient (Shiauchin Wang) that she would have to undergo an operation that same day and prepared her reports. The patient, although feeling slightly confused, assumed that the operation was advanced by one day. After a while, the transporter arrived at the obstetrics and gynecology department and asked for -patient Ms. Wang? (giving no other identifying information). Consequently, the wrong patient was brought to the OR suite.

408 29 Demonstration of System Usage Scenario 2

Wrong OR Event-While the wrong patient was brought to OR-5, the reader located in OR-5 detected the patient's identity and checked it with the OR schedule. Since the patient was not assigned to OR-5, the system displayed

410 identity and checked it with the OR schedule. Since the patient was not assigned to OR-411 a warning message bringing this fact to the nurse's attention (See Fig. 17).

412 **30** Fig.17. Warning message

Wrong-Site Surgery Event-Situations in which one doctor scheduled to perform an operation is substituted by another occur commonly in hospitals. However, whether a doctor is an attending physician or not, it is possible that he/she might memorize the wrong operation site; this is particularly true of substitute doctors who do not know the patient well.

Based on the scenario of wrong-site surgery, the system will automatically display the Ms. Wang's information including a chart on which the surgery site was marked while she was brought to OR-5 (See Fig. ??4). Therefore, the doctor was encouraged to review the displayed information and did not have to look for the paper-based chart.

Wrong-Patient Event-In the abovementioned situation, the patient -S hiau-ching Wang? probably underwent a wrong operation. However, with the RFID-based OR system, the nurse could be forced to reconfirm by using the admission application system. When the nurse assigned the RFID wristband to the wrong patient -Shia u-chin Wang,? the system asked for the patient's ID card number. After the system compared the patient's ID

424 card number with the OR schedule, a warning message would displayed (See Fig. 18).

425 **31** Fig.18 Warning message II

If the nurse incorrectly entered the ID card number of the correct patient -Shia u-ching Wang,? the system would 426 display the correct patient's information including the patient's picture (See Fig. 19). On seeing this displayed 427 picture, the nurse would realize that a mismatch exists in the results and would therefore take corrective action. 428 ??) actively provides patients' information to ensure that patients get correct procedures. The proposed system 429 decreases the probability of medical errors such as wrong patients, wrong locations, wrong medical staff and 430 wrong procedures. From the medical staff point of views, the system replaces some time-wasted manual input 431 processes. Therefore, it will improve operational efficiency in the OR and consequently help medical professionals 432 better manage patient care. 433

8

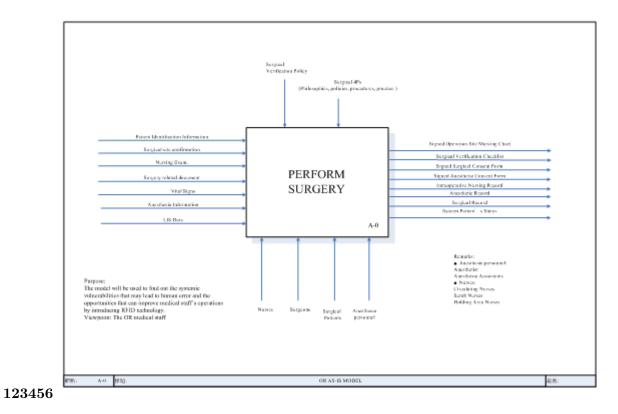


Figure 1: Fig. 1 .Fig. 2 .Fig. 3 .Fig. 4 .Fig. 5 .Fig. 6 .

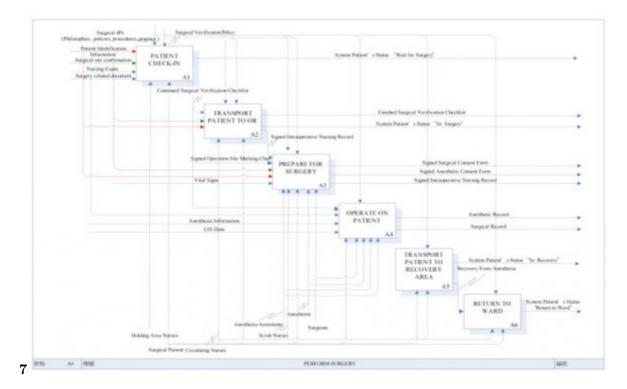


Figure 2: Fig. 7 .

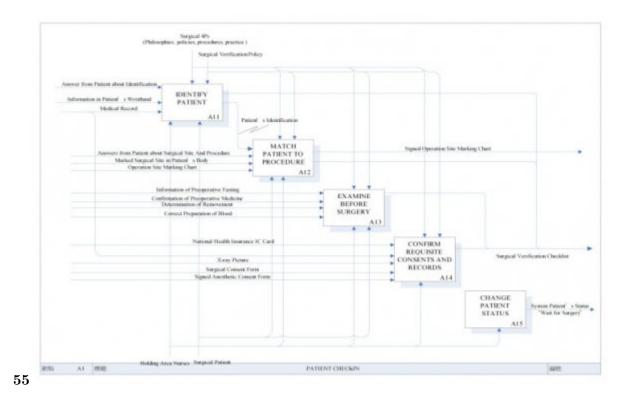


Figure 3: ? 5 5 ?

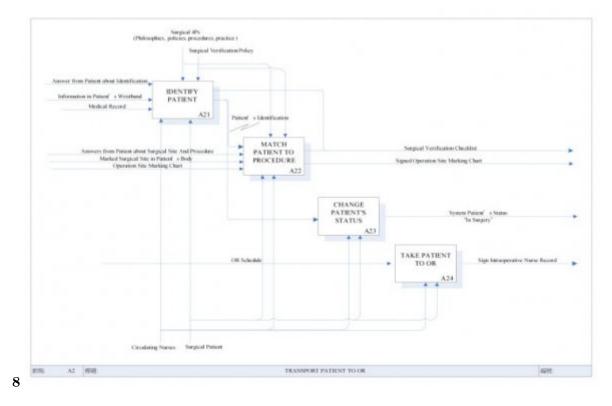


Figure 4: Fig. 8 .

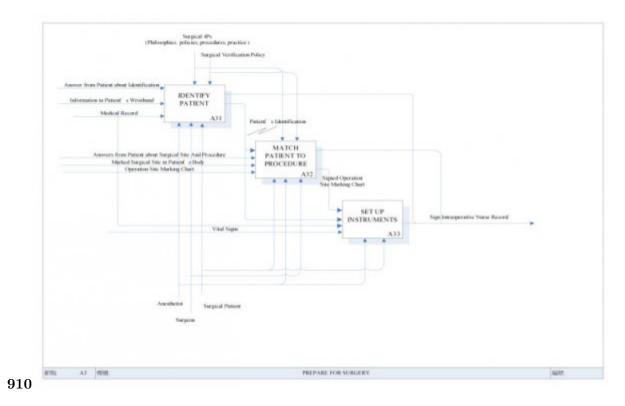


Figure 5: Fig. 9 . Fig. 10 .

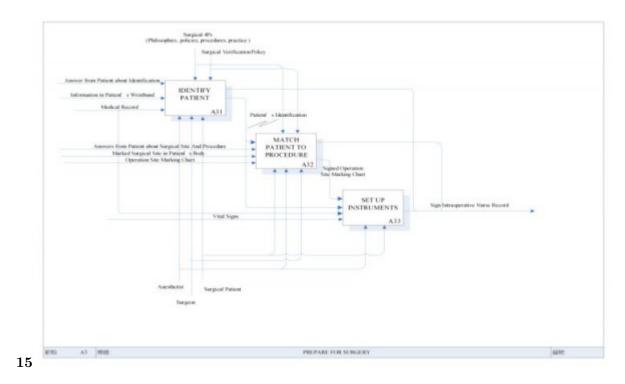


Figure 6: Fig. 15 .



Figure 7: Fig. 19

Failure to correctly identify patients constitutes one of the most serious risks to patient safety; however, in the OR, it can even cost a life. Entering the wrong OR-In general, a teaching medical center has numbers of contiguous ORs, each performing two to three cases daily. Moreover, OR schedule varies frequently. Hence, there are many opportunities for surgeons or patients to enter the wrong ORs. If a patient or a surgeon

enters a wrong OR without reconfirm, the event of wrong

[Note: Misidentification Of Patients-]

surgery could happen.

Figure 8:

- [Crossing the Quality Chasm: A New Health Care System for the 21st Century ()] Crossing theQuality 434
- Chasm: A New Health Care System for the 21st Century, 2001. Washington, DC: National Academy Press. 435 Institute of Medicine (Committee on Quality of Health Care in America)
- 436
- [Riley and Manias ()] 'Gatekeeping practices of nurses in operating rooms'. Robin Riley , Elizabeth Manias . 437 Social Science & Medicine 2009. 69 (2) p. . 438
- 439 [Makary et al. ()] 'Operating Room Briefings and Wrong-Site Surgery'. Martin A Makary, Arnab Mukherjee, J Bryan Sexton , Dora Syin , Emmanuelle Goodrich , Emily Hartmann , Lisa Rowen , Drew C Behrens , 440
- Michael Marohn, Peter J Pronovost. Journal of the American College of Surgeons 2007. 204 (2) p. . 441
- [Mendelsohn et al. ()] 'Patient Safety in Surgery'. Bsc Mendelsohn , Msc , M Md Bernstein , Mhsc . Israeli 442 Journal of Emergency Medicine 2009. 9 (2). 443
- [Seiden and Barach ()] S C Seiden, P Barach. Wrong-Side/Wrong-Site, Wrong-Procedure, and Wrong-Patient 444 Adverse Events, 2006. 141 p. . 445
- [Carstens et al. ()] 'Task analysis of healthcare delivery: A case study'. Deborah Carstens , Pauline Patterson , 446 Rosemary Laird, Paula Preston. Journal of Engineering and Technology Management 2009. 26 (1/2) p. . 447
- [Gawande et al. ()] 'The incidence and nature of surgical adverse events in Colorado and Utah in 1992'. A A 448 Gawande, E J Thomas, M J Zinner, T A Brennan. Surgery 1999. 126 (1) p. . 449
- [The Joint Commission: The Joint Commission Home Page] http://www.jointcommission.org/ The450 Joint Commission: The Joint Commission Home Page, 451
- [Kohn et al. ()] To Err is Human. Building a Safer Health System, L T Kohn, J M Corrigan, M S Donaldson. 452 2000. Washington, DC: National Academy Press. 453
- [Bates ()] 'Using information technology to improve surgical safety'. D W Bates . British journal of surgery 2004. 454
- 91 (8) p. . 455